


SUPPLEMENTARY MATERIAL

Preliminary Analytical Evaluation of the Automated Cobas i601 LC-MS/MS System for Immunosuppressants Quantification in a Clinical Laboratory

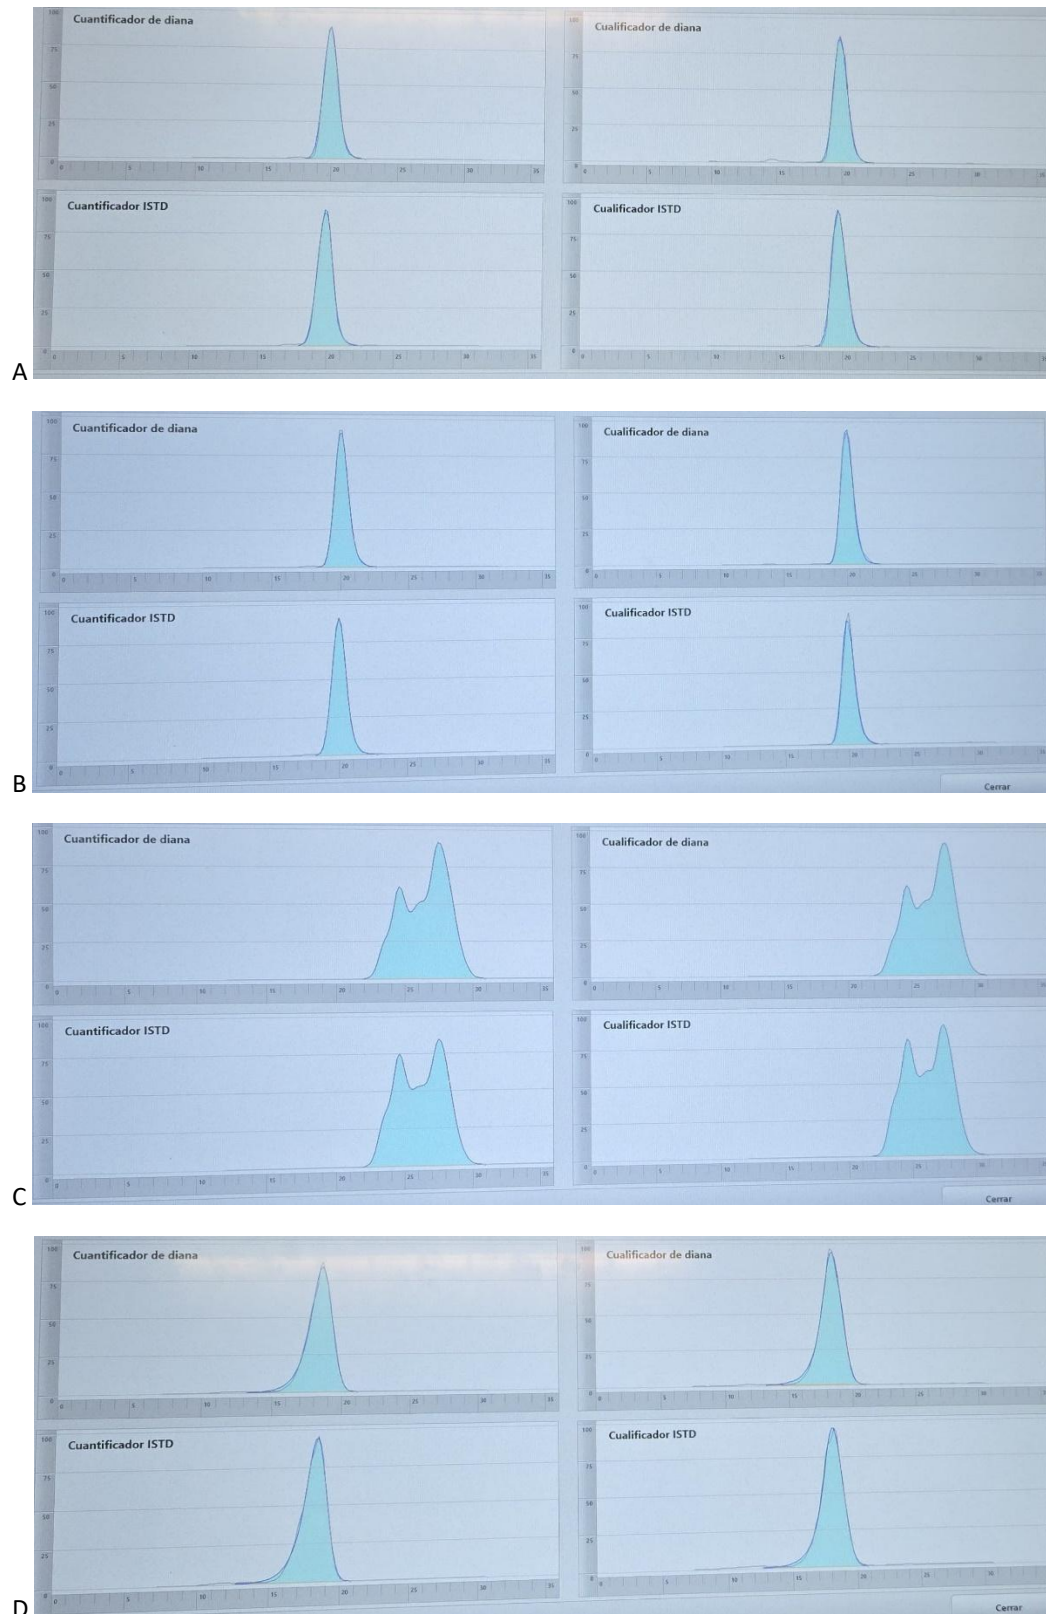

Supplementary Figure 1. Representative extracted ion chromatograms as displayed by the Cobas i601 system for A) sirolimus, B) everolimus, C) cyclosporine, and D) tacrolimus.